



TEST REPORT TUCHENG

Date: Jun. 16, 2020 Date of Receipt: May. 28, 2020

Report No.: TFF9E595 Quantity: 1PC Page Order/Pages: (P5/6) Ref. No.: NIL


Report Title: EMS Components Assembly Inc(PH004) Item: Mask

Address: 117-A Technology Avenue, Laguna Technopark, Inc. SEPZ, Binan, Laguna, 4024 Philippines

Test Items		Test Results	Test Methods
Microbial cleanliness (cfu/g)	1	3.9	EN 14683:2019
	2	3.9	EN ISO 11737-1:2018
	3	2.0	
	4	3.0	
	5	2.0	

Note: Sample description is given by the client: Surgical Mask N88

Note: The test report is the test results issued by the testing institution as requested by the consignor, it shall not determine the legitimacy of the product.

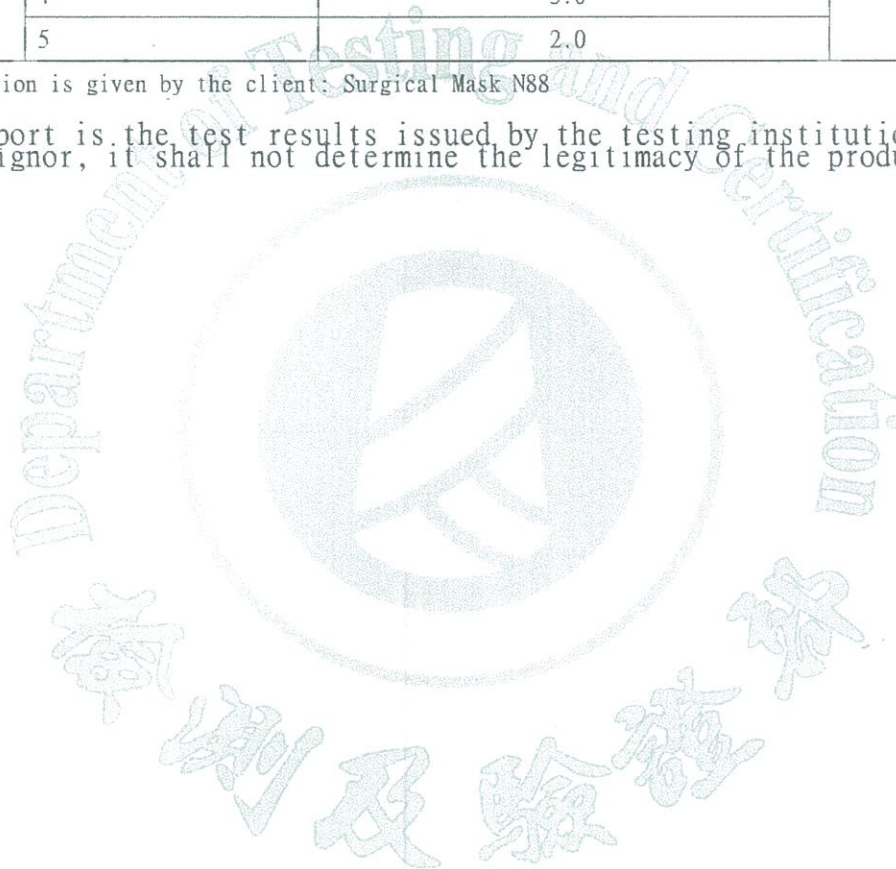

- Note:
1. This report is only responsible for the submitted sample(s), which will be kept for one month period.
  2. This report cannot be reproduced in any way, except in full context, without the prior approval in writing of this Department of Testing and Certification.
  3. The test report should not be used for public advertisement and commercial promotion.

Authorized by president of  
Taiwan Textile Research Institute

*Jui-hung kao*

Director,  
Department of Testing and  
Certification

Department of Testing and Certification, Taiwan Textile Research Institute  
No.6, Chengtian Rd., Tucheng Dist., New Taipei City 23674, Taiwan (R.O.C.)  
Tel : +886-2-22670321 ext. 7107, 7110  
Fax : +886-2-22675108, +886-2-22689839